

ILS Laboratories

8222 Vickers St, Suite 106, San Diego, CA 92111
(619) 329-3999 | ils-lab.com

Retatrutide - 15mg

Tested for: Nuvera Bioscience



COA #: COA-2026-PM2GZH
Lot Number: VP-RT15-26
Accession #: ACC-2026-13328
Labeled Content: 15mg

Analysis Date: 08/11/2026
Appearance: Good
Sample Matrix: Lyophilized
Date Received: 07/30/2026

PASS



Scan to verify
authenticity at ils-lab.com
Access Code: 68FRBPW5

Method: Purity, Identity & Quantitation (HPLC)

Identity	Peptide Purity	Fentanyl Free
Retatrutide	99.14%	


Purity, Identity & Quantitation (HPLC)

Analyte	Specification	Result	Unit	Status
Peptide Purity (HPLC)	>= 95.0%	99.14%	%	PASS
Net Peptide Content	Report Only	15.74	mg	N/A
Identity (HPLC-RTM)	Retatrutide	Confirmed	-	PASS
Fentanyl Screen	Immunoassay, 50 ng/mL cutoff	Not Detected	-	PASS



Retatrutide 15mg - VP-RT15-26

HPLC Chromatogram

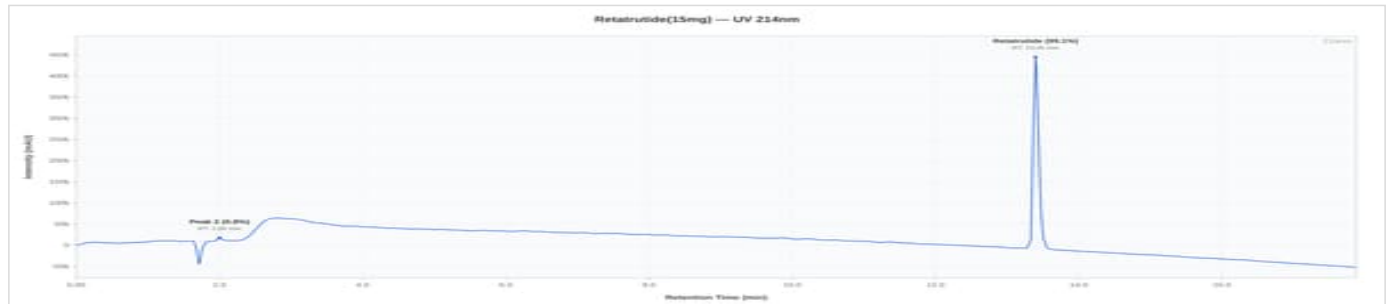

Retatrutide 15mg - VP-RT15-26: UV Chromatogram

Notes & Methodology

- Date Tested: 08/11/2026. Methods: Purity, Identity & Quantitation (HPLC).
- The sample was confirmed to be Retatrutide by HPLC. Identification by chromatographic retention time comparison with a reference standard.
- Peptide purity determined by RP-HPLC area normalization at 214 nm. Value represents the percentage of the target peptide relative to all peptide-related peaks. Non-peptide process-related impurities, if detected, are excluded from the calculation.
- Accreditation Scope: ILS Laboratories maintains ISO/IEC 17025 accreditation for activities listed in its published PJLA scope. Peptide testing reported on this certificate is performed for Research Use Only.
- This certificate reports analytical results for the sample(s) submitted to ILS Laboratories for testing. All sample identifications, product names, brand names, lot/batch numbers, and labeled content are provided by the submitting party and have not been independently verified. Results reflect only the analytical testing of the specific sample(s) provided and do not constitute an evaluation or endorsement of the manufacturer's processes, quality systems, or overall production. ILS Laboratories makes no representations regarding the intended use, safety, efficacy, regulatory status, or intellectual property ownership of any materials tested.



Issued by ILS Laboratories
(619) 329-3999
ils-lab.com



Dr. Greg Kalyuzhny
Lab Director
08/11/2026

COA #: COA-2026-PM2GZH
Access Code: 68FRBPW5
Verify: portal.ils-lab.com/verify/Wa-sCUSdeMfgTS6X
Issued: 08/11/2026

ILS Laboratories

8222 Vickers St, Suite 106, San Diego, CA 92111
(619) 329-3999 | ils-lab.com

Retatrutide - 20mg

Tested for: Nuvera Bioscience



COA #: COA-2026-JR1V3O
Lot Number: VP-RT20-26
Accession #: ACC-2026-13329
Labeled Content: 20mg

Analysis Date: 08/11/2026
Appearance: Good
Sample Matrix: Lyophilized
Date Received: 07/30/2026

PASS



Scan to verify
authenticity at ils-lab.com
Access Code: 7EVN47VA

Method: Purity, Identity & Quantitation (HPLC)

Identity	Peptide Purity	Fentanyl Free
Retatrutide	98.99%	


Purity, Identity & Quantitation (HPLC)

Analyte	Specification	Result	Unit	Status
Peptide Purity (HPLC)	>= 95.0%	98.99%	%	PASS
Net Peptide Content	Report Only	20.83	mg	N/A
Identity (HPLC-RTM)	Retatrutide	Confirmed	-	PASS
Fentanyl Screen	Immunoassay, 50 ng/mL cutoff	Not Detected	-	PASS



Retatrutide 20mg -
VP-RT20-26

HPLC Chromatogram

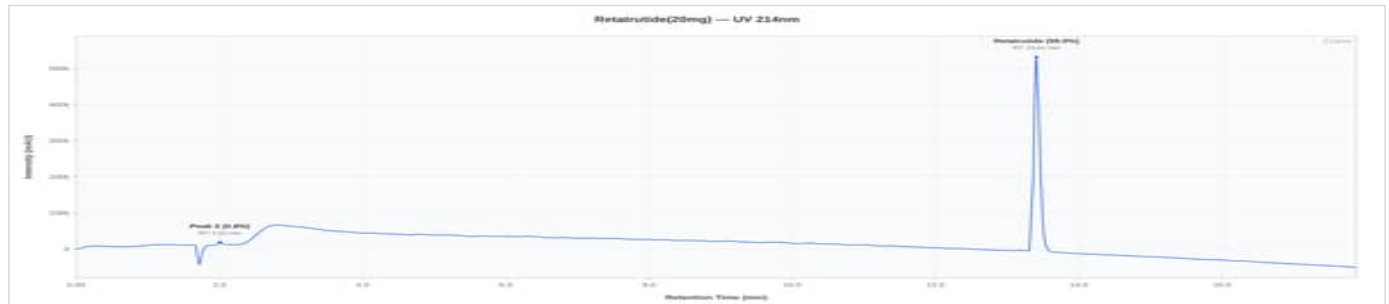

Retatrutide 20mg - VP-RT20-26: UV Chromatogram

Notes & Methodology

- Date Tested: 08/11/2026. Methods: Purity, Identity & Quantitation (HPLC).
- The sample was confirmed to be Retatrutide by HPLC. Identification by chromatographic retention time comparison with a reference standard.
- Peptide purity determined by RP-HPLC area normalization at 214 nm. Value represents the percentage of the target peptide relative to all peptide-related peaks. Non-peptide process-related impurities, if detected, are excluded from the calculation.
- Accreditation Scope: ILS Laboratories maintains ISO/IEC 17025 accreditation for activities listed in its published PJLA scope. Peptide testing reported on this certificate is performed for Research Use Only.
- This certificate reports analytical results for the sample(s) submitted to ILS Laboratories for testing. All sample identifications, product names, brand names, lot/batch numbers, and labeled content are provided by the submitting party and have not been independently verified. Results reflect only the analytical testing of the specific sample(s) provided and do not constitute an evaluation or endorsement of the manufacturer's processes, quality systems, or overall production. ILS Laboratories makes no representations regarding the intended use, safety, efficacy, regulatory status, or intellectual property ownership of any materials tested.



Issued by ILS Laboratories
(619) 329-3999
ils-lab.com



Dr. Greg Kalyuzhny
Lab Director
08/11/2026

COA #: COA-2026-JR1V3O
Access Code: 7EVN47VA
Verify: portal.ils-lab.com/verify/YZW4Gp7t17GfZpQ
Issued: 08/11/2026

ILS Laboratories

8222 Vickers St, Suite 106, San Diego, CA 92111
(619) 329-3999 | ils-lab.com

Retatrutide - 30mg

Tested for: Nuvera Bioscience



COA #: COA-2026-OSZLOP
Lot Number: VP-RT30-26
Accession #: ACC-2026-13330
Labeled Content: 30mg

Analysis Date: 08/11/2026
Appearance: Good
Sample Matrix: Lyophilized
Date Received: 07/30/2026

PASS



Scan to verify
authenticity at ils-lab.com
Access Code: L29DRKHL

Method: Purity, Identity & Quantitation (HPLC)

Identity	Peptide Purity	Fentanyl Free
Retatrutide	99.03%	


Purity, Identity & Quantitation (HPLC)

Analyte	Specification	Result	Unit	Status
Peptide Purity (HPLC)	>= 95.0%	99.03%	%	PASS
Net Peptide Content	Report Only	30.47	mg	N/A
Identity (HPLC-RTM)	Retatrutide	Confirmed	-	PASS
Fentanyl Screen	Immunoassay, 50 ng/mL cutoff	Not Detected	-	PASS



Retatrutide 30mg -
VP-RT30-26

HPLC Chromatogram

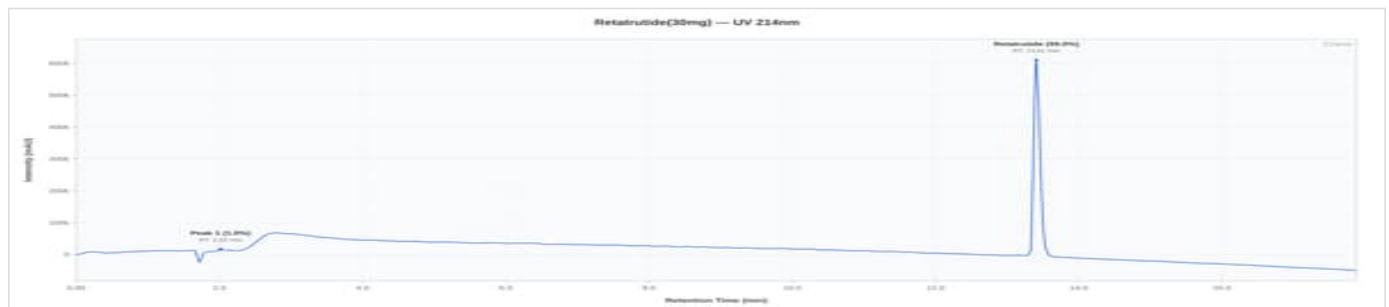

Retatrutide 30mg - VP-RT30-26: UV Chromatogram

Notes & Methodology

- Date Tested: 08/11/2026. Methods: Purity, Identity & Quantitation (HPLC).
- The sample was confirmed to be Retatrutide by HPLC. Identification by chromatographic retention time comparison with a reference standard.
- Peptide purity determined by RP-HPLC area normalization at 214 nm. Value represents the percentage of the target peptide relative to all peptide-related peaks. Non-peptide process-related impurities, if detected, are excluded from the calculation.
- Accreditation Scope: ILS Laboratories maintains ISO/IEC 17025 accreditation for activities listed in its published PJLA scope. Peptide testing reported on this certificate is performed for Research Use Only.
- This certificate reports analytical results for the sample(s) submitted to ILS Laboratories for testing. All sample identifications, product names, brand names, lot/batch numbers, and labeled content are provided by the submitting party and have not been independently verified. Results reflect only the analytical testing of the specific sample(s) provided and do not constitute an evaluation or endorsement of the manufacturer's processes, quality systems, or overall production. ILS Laboratories makes no representations regarding the intended use, safety, efficacy, regulatory status, or intellectual property ownership of any materials tested.



Issued by ILS Laboratories
(619) 329-3999
ils-lab.com



Dr. Greg Kalyuzhny
Lab Director
08/11/2026

COA #: COA-2026-OSZLOP
Access Code: L29DRKHL
Verify: portal.ils-lab.com/verify/xA-Uk6ZvhE9BNH7j
Issued: 08/11/2026